


# HPLC Analysis of Lidocaine/Prilocaine Formulations

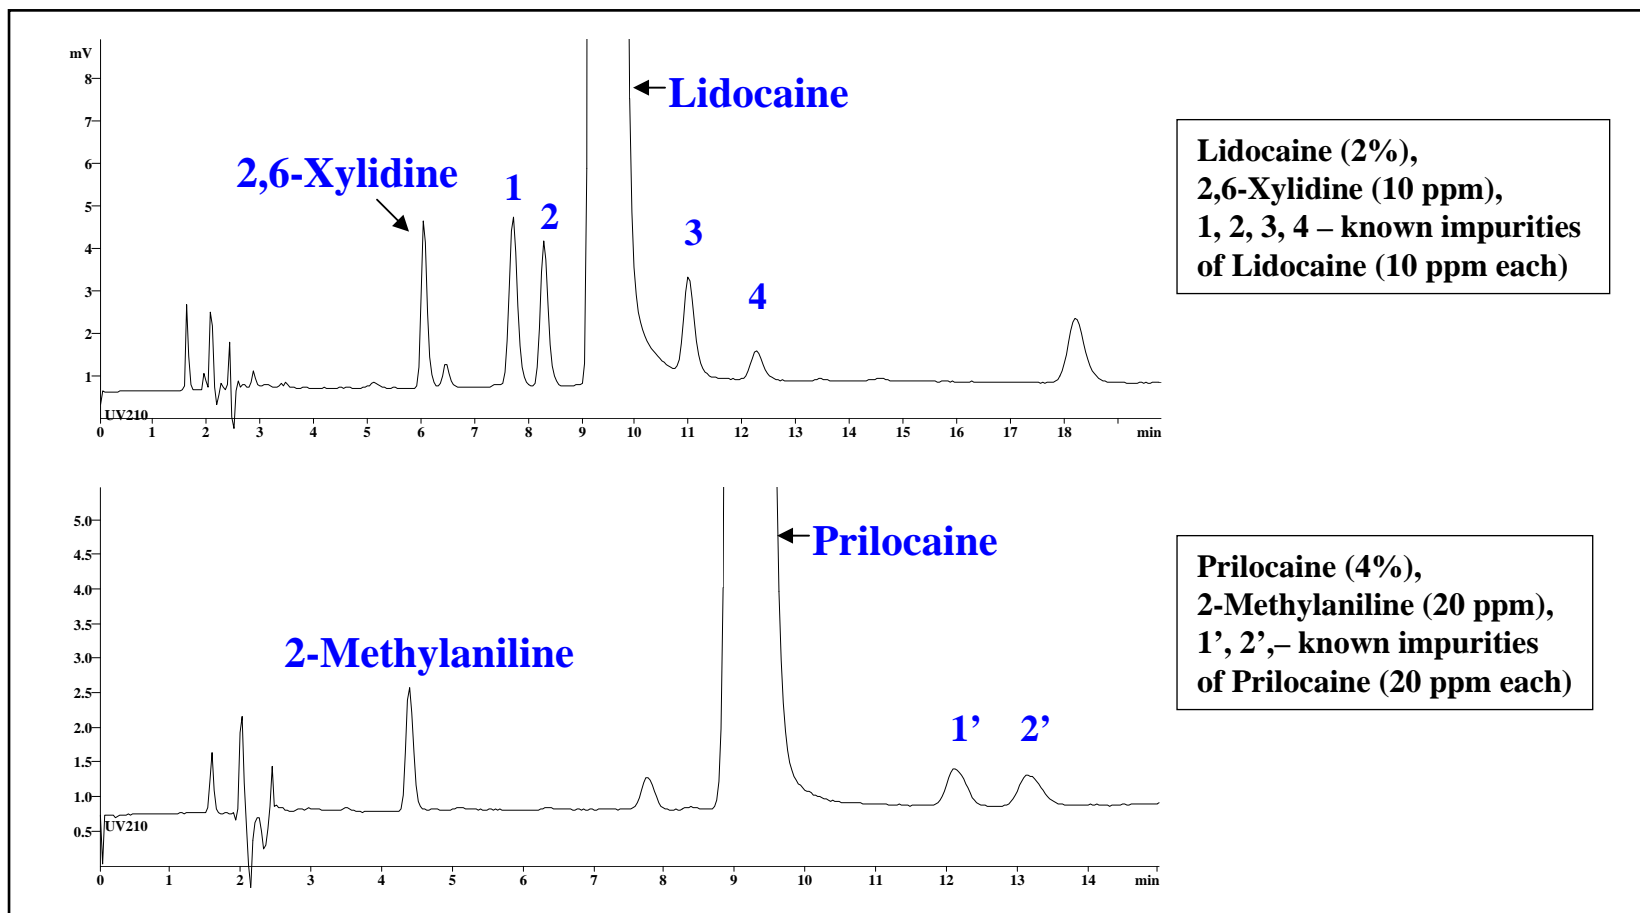

**HPLC analysis of Lidocaine and Prilocaine formulations.  
Detector: UV-Vis, 210 nm.**